

Fig. 1

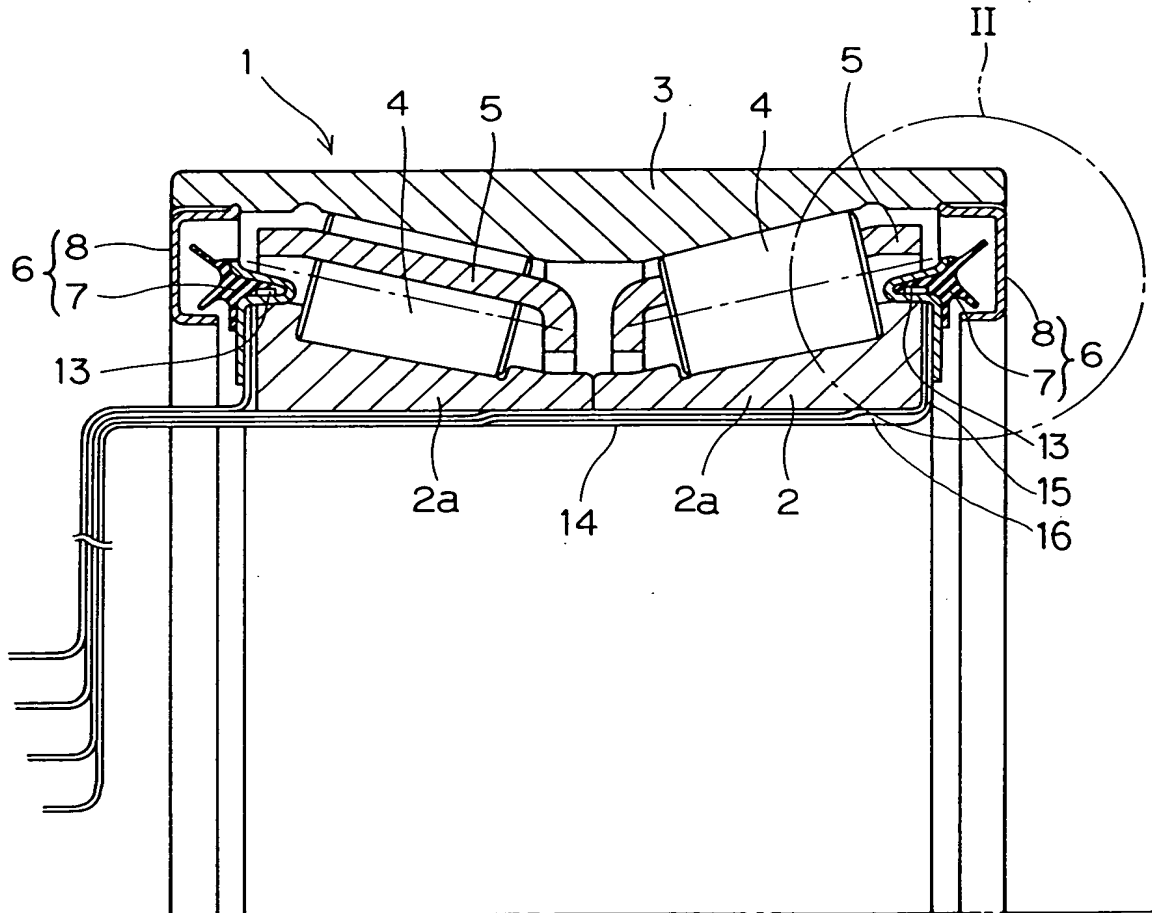


Fig. 1 is a cross-sectional view of the device.

Fig. 2

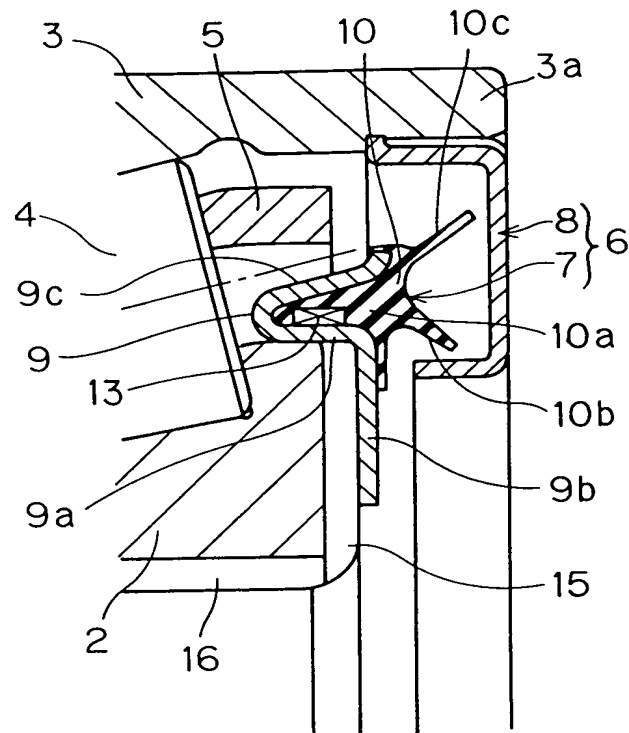


Fig. 3

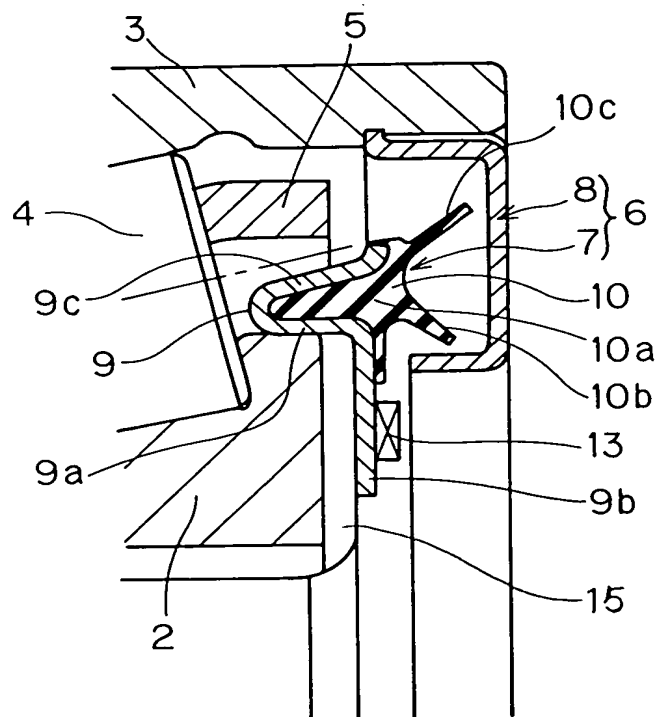


Fig. 4

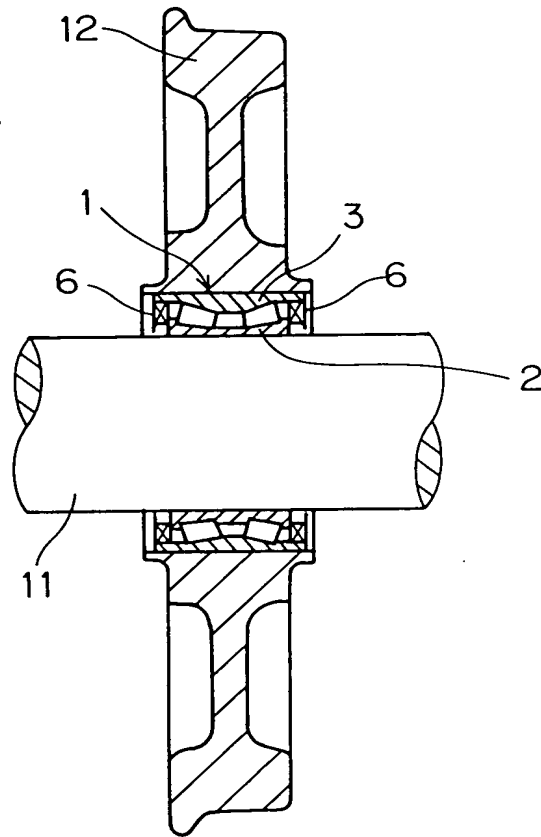


Fig. 5

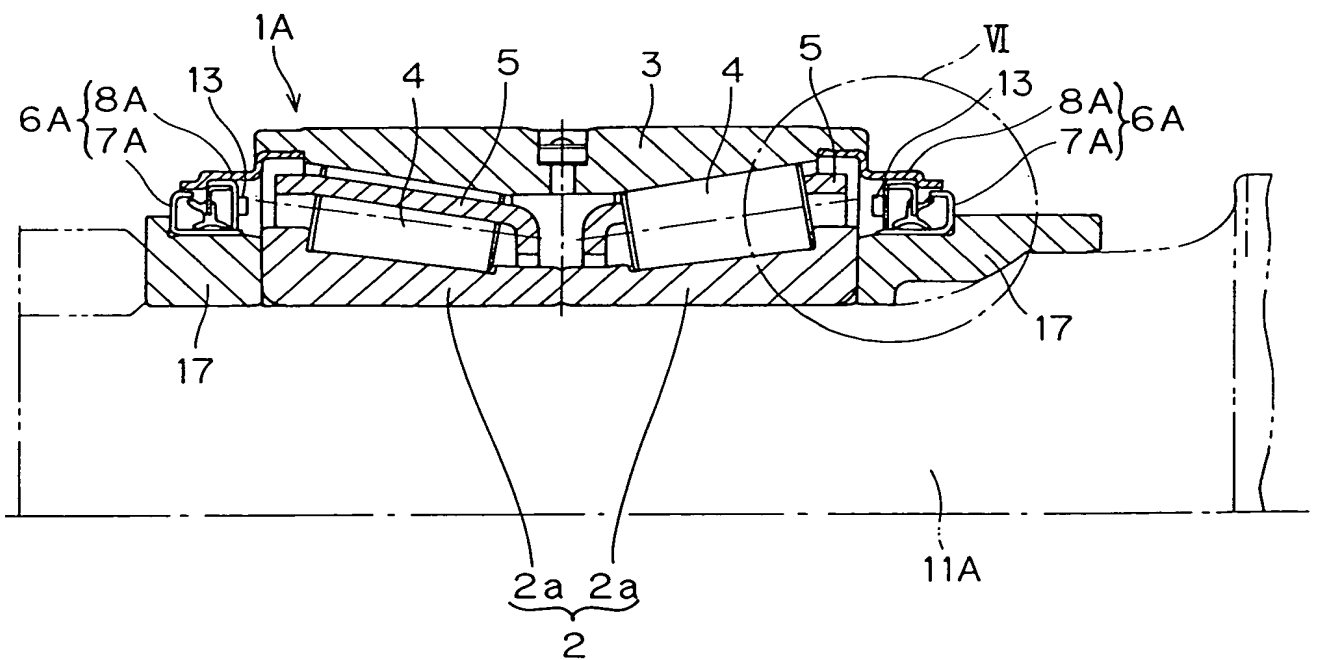


Fig. 6

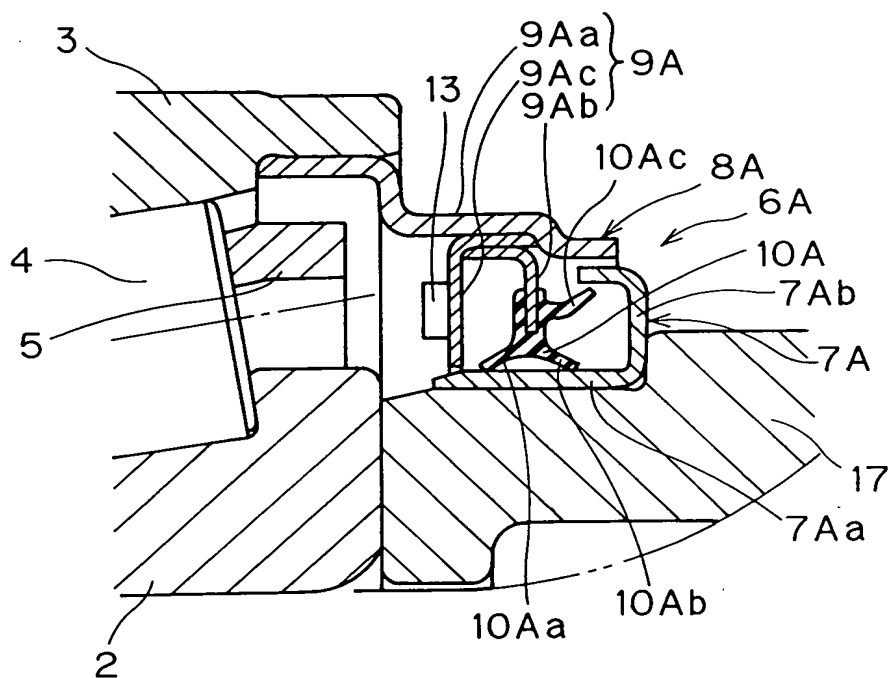


Fig. 7

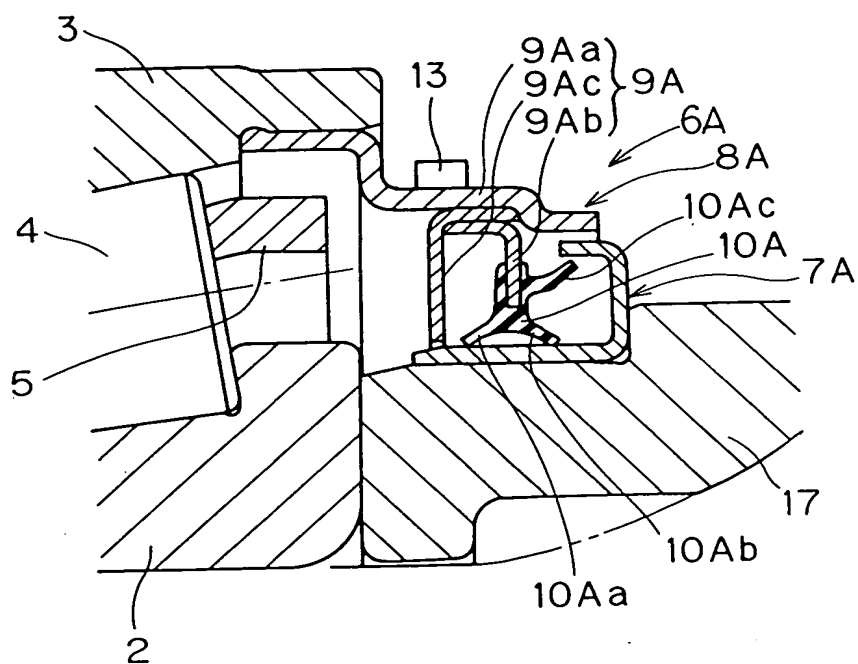


Fig. 8

